


Instructions for Use




1 Clean test site with isopropyl alcohol and air dry. Remove protective cap from safety lancet.

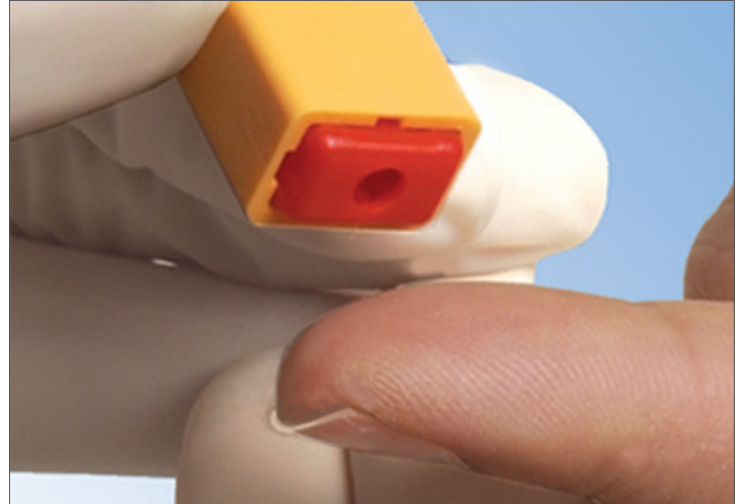

2 Place red end of safety lancet on the test site.



3 Push the safety lancet down against test site to activate lancet mechanism.

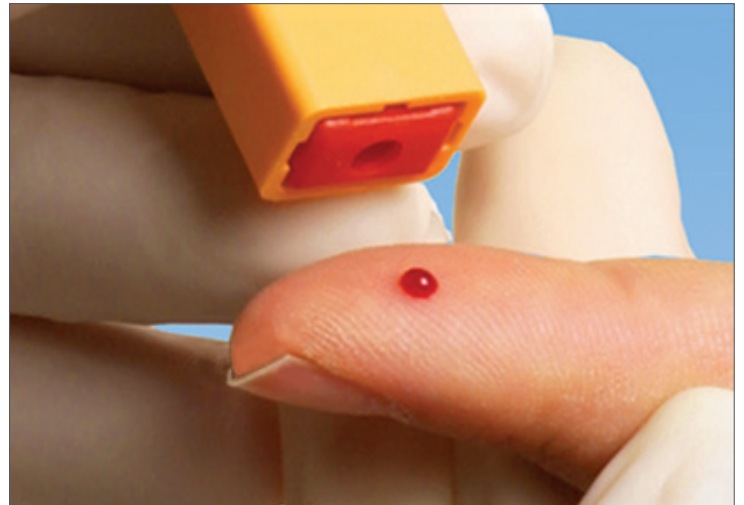

4 Once used, simply discard lancet into a sharps container.

Single-use only. Reuse may result in patient cross-contamination.

[medipurpose.com/surgilance/ifu/](https://www.medipurpose.com/surgilance/ifu/)